

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01070	Calib. Date: 09/15/2014
Certification File No.:	01071	Calib. No.: 00024
Linearity File No.:	01072	Cert. Date: 09/15/2014
Solution File No.:	01104	Cert. No.: 00017
Sequential File No.:	01104	Lin. Date: 09/15/2014
		Lin. No.: 00017
		Soln. Date: 02/14/2015
		Soln. No.: 00201
		File Date: 02/14/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWL S3-0440
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 0754

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:32S		
Control 1 EC	0.097%	01:33S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	01:33S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:34S		
Control 2 EC	0.098%	01:34S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:35S		
Control 3 EC	0.099%	01:36S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	01:36S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:37S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DIFABIO

First Name: LANCE

MI: S

Signature: _____

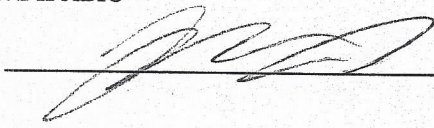

Badge No.: 3431

Date: 02/14/2015