

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01261 **Calib. Date:** 03/01/2016 **Calib. No.:** 00029
Certification File No.: 01262 **Cert. Date:** 03/01/2016 **Cert. No.:** 00021
Linearity File No.: 01263 **Lin. Date:** 03/01/2016 **Lin. No.:** 00021
Solution File No.: 01294 **Soln. Date:** 05/01/2016 **Soln. No.:** 00230
Sequential File No.: 01294 **File Date:** 05/01/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWL S3-0441
Control Solution %: 0.100% **Expires:** 06/13/2017
Solution Control Lot: 15F139 **Bottle No.:** 0723

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:23D		
Control 1 EC	0.096%	00:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	00:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:24D		
Control 2 EC	0.096%	00:25D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	00:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:26D		
Control 3 EC	0.095%	00:26D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	00:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:27D		

All tests within acceptable tolerance.

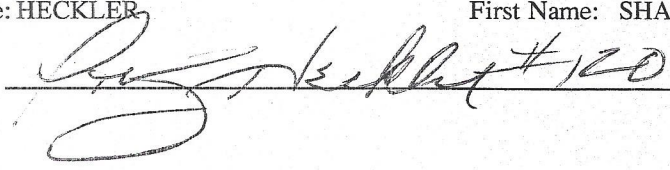
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: 

Badge No.: 120

Date: 05/01/2016