

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01348	Calib. Date: 10/28/2016
Certification File No.:	01349	Calib. No.: 00032
Linearity File No.:	01350	Cert. Date: 10/28/2016
Solution File No.:	01410	Cert. No.: 00023
Sequential File No.:	01410	Lin. Date: 10/28/2016
		Lin. No.: 00023
		Soln. Date: 03/17/2017
		Soln. No.: 00247
		File Date: 03/17/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWL S3-0440
Solution Control Lot:	16390	Expires: 12/02/2018
		Bottle No.: 1136

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:16S		
Control 1 EC	0.097%	07:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	07:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:18S		
Control 2 EC	0.094%	07:19S	33.9°C	CONTROL TEST FAILED
Control 2 IR	0.091%	07:19S	33.9°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	07:19S		
Control 3 EC	0.096%	07:20S	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.092%	07:20S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	07:21S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: _____

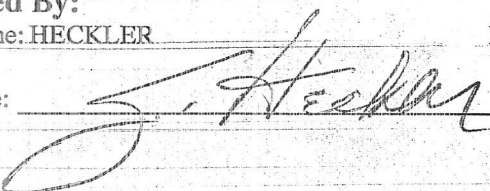

Badge No.: 120

Date: 03/17/2017