

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01739	Calib. Date: 06/21/2019
Certification File No.:	01740	Calib. No.: 00039
Linearity File No.:	01741	Cert. Date: 06/21/2019
Solution File No.:	01773	Cert. No.: 00030
Sequential File No.:	01773	Lin. Date: 06/21/2019
		Lin. No.: 00030
		Soln. Date: 11/01/2019
		Soln. No.: 00299
		File Date: 11/01/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWL S3-0441
Solution Control Lot:	19020	Expires: 01/08/2021
		Bottle No.: 1143

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:04S		
Control 1 EC	0.101%	03:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:05S		
Control 2 EC	0.099%	03:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:06S		
Control 3 EC	0.099%	03:07S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:08S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: \_\_\_\_\_

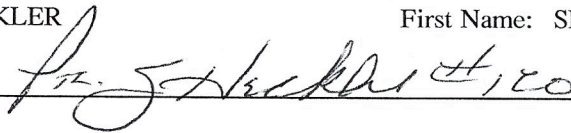

Badge No.: 120

Date: 11/01/2019