

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01775	Calib. Date: 11/27/2019
Certification File No.:	01776	Calib. No.: 00040
Linearity File No.:	01777	Cert. Date: 11/27/2019
Solution File No.:	01794	Cert. No.: 00031
Sequential File No.:	01794	Lin. Date: 11/27/2019
		Lin. No.: 00031
		Soln. Date: 02/15/2020
		Soln. No.: 00304
		File Date: 02/15/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWL S3-0440
Solution Control Lot:	19020	Expires: 01/08/2021
		Bottle No.: 1151

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:45S		
Control 1 EC	0.098%	17:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:47S		
Control 2 EC	0.098%	17:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:48S		
Control 3 EC	0.098%	17:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:50S		

All tests within acceptable tolerance.

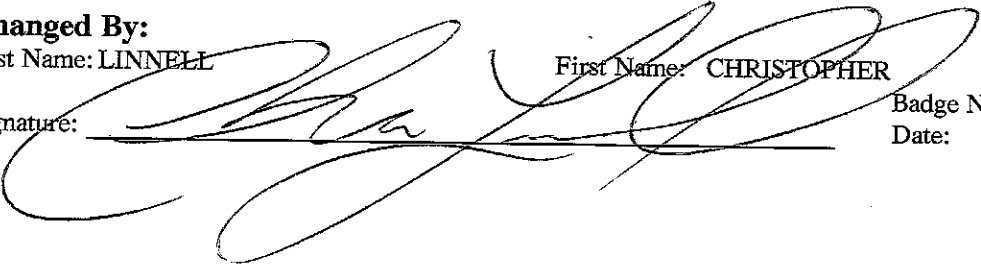
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 02/15/2020