

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01775 Calib. Date: 11/27/2019 Calib. No.: 00040
Certification File No.: 01776 Cert. Date: 11/27/2019 Cert. No.: 00031
Linearity File No.: 01777 Lin. Date: 11/27/2019 Lin. No.: 00031
Solution File No.: 01801 Soln. Date: 03/07/2020 Soln. No.: 00305
Sequential File No.: 01801 File Date: 03/07/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0440
Control Solution %: 0.100% Expires: 01/08/2021
Solution Control Lot: 19020 Bottle No.: 1417

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:45S		
Control 1 EC	0.097%	17:46S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	17:46S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:47S		
Control 2 EC	0.097%	17:48S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	17:48S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:48S		
Control 3 EC	0.097%	17:49S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:50S		

All tests within acceptable tolerance.

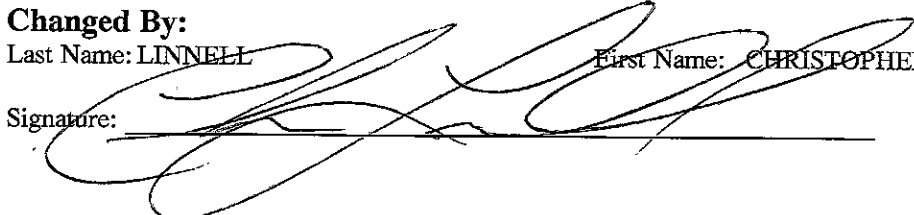
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 03/07/2020