

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01848 Calib. Date: 09/29/2020 Calib. No.: 00042
Certification File No.: 01849 Cert. Date: 09/29/2020 Cert. No.: 00033
Linearity File No.: 01850 Lin. Date: 09/29/2020 Lin. No.: 00033
Solution File No.: 01874 Soln. Date: 03/04/2021 Soln. No.: 00326
Sequential File No.: 01874 File Date: 03/04/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0440
Control Solution %: 0.100% Expires: 01/13/2023
Solution Control Lot: 21010 Bottle No.: 0506

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:37S		
Control 1 EC	0.101%	20:37S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38S		
Control 2 EC	0.100%	20:39S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:40S		
Control 3 EC	0.099%	20:40S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:41S		

All tests within acceptable tolerance.

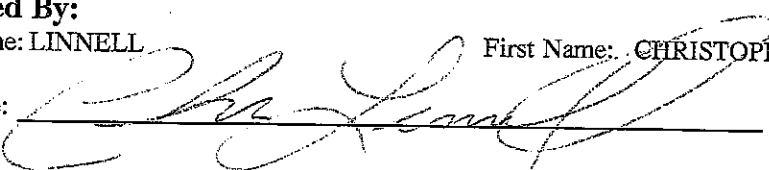
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 03/04/2021