

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01923	Calib. Date: 07/27/2021
Certification File No.:	01924	Calib. No.: 00044
Linearity File No.:	01925	Cert. Date: 07/27/2021
Solution File No.:	01957	Cert. No.: 00035
Sequential File No.:	01957	Lin. Date: 07/27/2021
		Lin. No.: 00035
		Soln. Date: 10/18/2021
		Soln. No.: 00338
		File Date: 10/18/2021

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWL S3-0440
Control Solution %:	0.100%		Expires: 01/13/2023
Solution Control Lot:	21010		Bottle No.: 0165

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:10D		
Control 1 EC	0.101%	14:11D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:12D		
Control 2 EC	0.099%	14:12D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:13D		
Control 3 EC	0.099%	14:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: _____

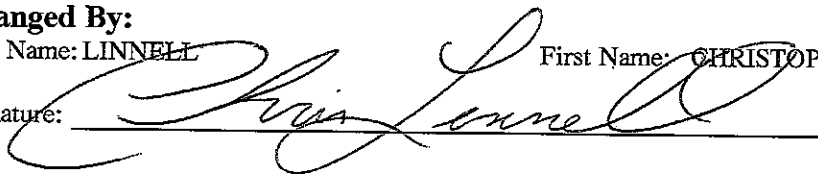

Badge No.: 128

Date: 10/18/2021