

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01975	Calib. Date: 01/20/2022
Certification File No.:	01976	Calib. No.: 00045
Linearity File No.:	01977	Cert. Date: 01/20/2022
Solution File No.:	02011	Cert. No.: 00036
Sequential File No.:	02011	Lin. Date: 01/20/2022
		Lin. No.: 00036
		Soln. Date: 04/04/2022
		Soln. No.: 00346
		File Date: 04/04/2022

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWL S3-0441
Control Solution %: 0.100%		Expires: 12/28/2023
Solution Control Lot: 21480		Bottle No.: 0240

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:29D		
Control 1 EC	0.098%	13:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:31D		
Control 2 EC	0.097%	13:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:32D		
Control 3 EC	0.097%	13:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: _____

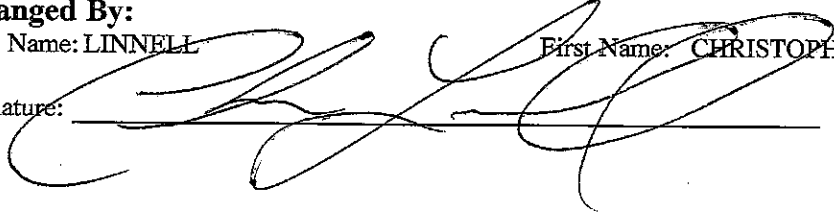

Badge No.: 128

Date: 04/04/2022