

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWJ-0018  
Location: SEASIDE HEIGHTS POLICE  
Calibration File No.: 01975 Calib. Date: 01/20/2022 Calib. No.: 00045  
Certification File No.: 01976 Cert. Date: 01/20/2022 Cert. No.: 00036  
Linearity File No.: 01977 Lin. Date: 01/20/2022 Lin. No.: 00036  
Solution File No.: 02046 Soln. Date: 06/04/2022 Soln. No.: 00349  
Sequential File No.: 02046 File Date: 06/04/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0441  
Control Solution %: 0.100% Expires: 12/28/2023  
Solution Control Lot: 21480 Bottle No.: 0321

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:59D		
Control 1 EC	0.097%	14:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	14:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:00D		
Control 2 EC	0.097%	15:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:02D		
Control 3 EC	0.098%	15:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	15:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:03D		

All tests within acceptable tolerance.

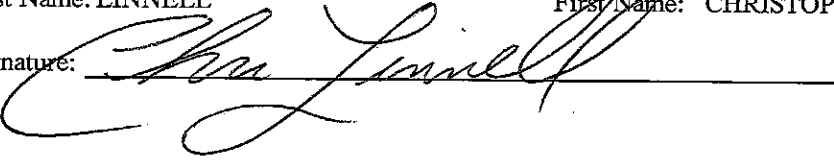
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 06/04/2022