

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	02070	Calib. Date: 07/15/2022
Certification File No.:	02071	Calib. No.: 00046
Linearity File No.:	02072	Cert. Date: 07/15/2022
Solution File No.:	02080	Cert. No.: 00037
Sequential File No.:	02080	Lin. Date: 07/15/2022
		Lin. No.: 00037
		Soln. Date: 07/30/2022
		Soln. No.: 00353
		File Date: 07/30/2022

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWL S3-0440
Control Solution %: 0.100%		Expires: 12/28/2023
Solution Control Lot: 21480		Bottle No.: 0449

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:21D		
Control 1 EC	0.099%	20:22D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:23D		
Control 2 EC	0.099%	20:23D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:24D		
Control 3 EC	0.099%	20:25D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: \_\_\_\_\_

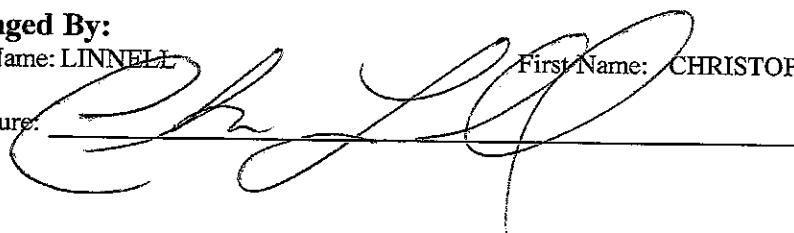

Badge No.: 128

Date: 07/30/2022