

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	02070	Calib. Date:	07/15/2022
Certification File No.:	02071	Cert. Date:	07/15/2022
Linearity File No.:	02072	Lin. Date:	07/15/2022
Solution File No.:	02113	Soln. Date:	11/20/2022
Sequential File No.:	02113	File Date:	11/20/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWL S3-0440
Solution Control Lot:	22160	Expires:	05/09/2024
		Bottle No.:	1005

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:03S		
Control 1 EC	0.101%	20:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:05S		
Control 2 EC	0.099%	20:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:06S		
Control 3 EC	0.099%	20:07S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:08S		

All tests within acceptable tolerance.

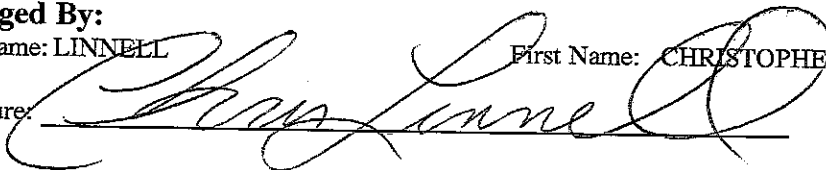
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 11/20/2022