

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	02156	Calib. Date: 05/31/2023
Certification File No.:	02157	Calib. No.: 00048
Linearity File No.:	02158	Cert. Date: 05/31/2023
Solution File No.:	02167	Cert. No.: 00039
Sequential File No.:	02167	Lin. Date: 05/31/2023
		Lin. No.: 00039
		Soln. Date: 06/25/2023
		Soln. No.: 00367
		File Date: 06/25/2023

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWL S3-0440
Control Solution %:	0.100%		Expires: 05/09/2024
Solution Control Lot:	22160		Bottle No.: 0896

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:55D		
Control 1 EC	0.100%	21:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:56D		
Control 2 EC	0.099%	21:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:58D		
Control 3 EC	0.099%	21:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BOYD

First Name: JAMES

MI: T

Signature: _____

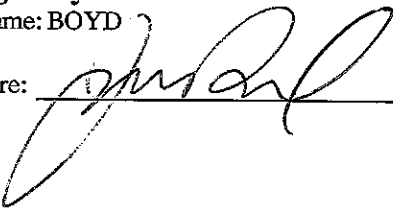

Badge No.: 4332

Date: 06/25/2023