

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	02156	Calib. Date: 05/31/2023
Certification File No.:	02157	Calib. No.: 00048
Linearity File No.:	02158	Cert. Date: 05/31/2023
Solution File No.:	02174	Cert. No.: 00039
Sequential File No.:	02174	Lin. Date: 05/31/2023
		Lin. No.: 00039
		Soln. Date: 07/04/2023
		Soln. No.: 00368
		File Date: 07/04/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWL S3-0440
Solution Control Lot:	23010	Expires: 01/11/2025
		Bottle No.: 1131

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:16D		
Control 1 EC	0.100%	11:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		
Control 2 EC	0.100%	11:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	11:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:19D		
Control 3 EC	0.100%	11:19D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.102%	11:19D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature:

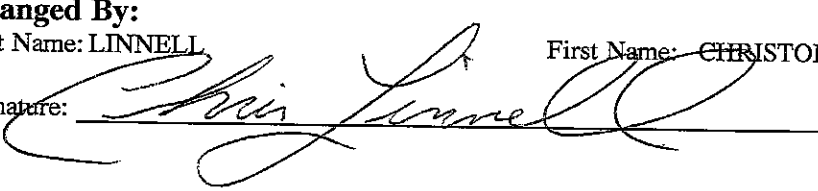

Badge No.: 128

Date: 07/04/2023