

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 02203 Calib. Date: 09/29/2023 Calib. No.: 00049
Certification File No.: 02204 Cert. Date: 09/29/2023 Cert. No.: 00040
Linearity File No.: 02205 Lin. Date: 09/29/2023 Lin. No.: 00040
Solution File No.: 02212 Soln. Date: 10/31/2023 Soln. No.: 00373
Sequential File No.: 02212 File Date: 10/31/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0440
Control Solution %: 0.100% Expires: 09/12/2025
Solution Control Lot: 23330 Bottle No.: 0156

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:38S		
Control 1 EC	0.101%	16:38S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:38S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:39S		
Control 2 EC	0.099%	16:40S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:40S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:40S		
Control 3 EC	0.099%	16:41S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature:

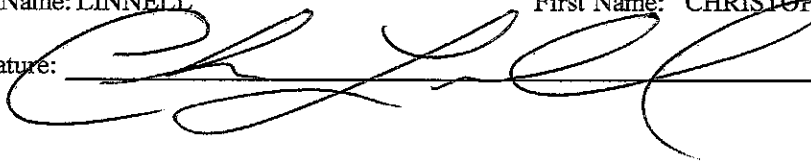

Badge No.: 128

Date: 10/31/2023