

## ALCOTEST 9510 PARAMETER REPORT

### Equipment

Serial No.: ARMK-0265  
Firmware: 8326739 1.5  
WinCE application: 8326738 2.9  
Configuration: 8326737 3.10

Date: 02/26/2026  
Time: 15:56:29

### Parameter

min. blow time	5.0	s
min. breath volume for females of age 60+	1.2	L
min. breath volume for all other	1.5	L
min. blow flow	4.5	L/min
plateau detection limit	4	%
plateau detection start conc.	70	microgram/L
neg. flow detection (part. vacuum)	10.0	hPa
neg. flow detection sensitivity	10	
cal. gas abort volume	0.4	L
result-to-zero limit	0.0050	%BAC
ambient air check limit	0.0049	%BAC
interference det. d-criterion limit abs.	38	microgram/L
interference det. d-criterion limit rel.	10.0	%
interference det. t-criterion limit abs.	8	microgram/L
interference det. t-criterion limit rel.	2.1	%
IR CO2 offset	10	microgram/L
IR H2O offset	4	microgram/L
EC H2O offset	0	microgram/L
Value-based EC aging comp. on/off (1/0)	0	
Time-based EC aging comp. on/off (1/0)	1	
Time-based EC aging comp. per month	0.2	%
Time-based EC aging comp. maximum	3.0	%
EC fatigue comp. max. sum	15000	
EC fatigue comp. factor	50	
EC fatigue comp. minutes	180	
mouth alc. mark limit	500	
mouth alc. lower limit	30	
mouth alc. slope	6	
mouth alc. zero limit	50	
mouth alc. max. neg. sum	6	
mouth alc. max. 2nd derivative	35	

**ALCOTEST 9510 CERTIFICATION REPORT - WET ADJUST (PART I)**  
*Seaside Heights*

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Wet Adjust Record**

Wet Adjust File No.: 208 Wet Adjust Date: 02/26/2026 Wet Adjust No.: 7  
Wet Adjust Time: 16:37:34

Concentration: 0.100 %  
Adjusting Unit: X-Cal 2000 Adj. Unit Ser. No.: ARRC-0011 Adj. Unit Exp.: 08/19/2026  
Solution Lot No.: 25180 Soln. Bottle No.: 149 Adjust Soln. Exp.: 06/03/2027

Preadjust Simulator Temp.: 34.00 degree C  
Postadjust Simulator Temp.: 34.01 degree C

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Bellay - First Name: David MI: M. Badge No.: 8112

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*David Bellay 8112*

Signed:

Date: 02/26/2026

ID: 50

**ALCOTEST 9510 CERTIFICATION REPORT - DRY ADJUST (PART II)**  
*Seaside Heights*

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Dry Adjust Record**

Dry Adjust File No.: 209 Dry Adjust Date: 02/26/2026 Dry Adjust No.: 7  
Dry Adjust Time: 16:55:58

Concentration: 0.100 %  
Dry Gas Lot No.: 302-402755160 Adjust Gas Exp.: 05/24/2026  
Barom. Model No.: Mensor CPG2300 Barom. Serial No.: 41001275 Barom. Cert. Exp.: 08/23/2026  
Pre-adjust Amb. Pressure: 1011 hPa Post-adjust Amb. Pressure: 1011 hPa

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Bellay - First Name: David MI: M. Badge No.: 8112

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.



Signed:

Date: 02/26/2026

ID: 50

**ALCOTEST 9510 CERTIFICATION REPORT - LINEARITY (PART III)**  
*Seaside Heights*

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Linearity Record**

Linearity File No.: 210 Lin. Date: 02/26/2026 Lin. No.: 7

0.040% Dry Gas Lot No.: 302-402730318 Adjust. Gas Exp.: 04/27/2026  
0.080% Dry Gas Lot No.: 302-402732434 Adjust. Gas Exp.: 04/28/2026  
0.160% Dry Gas Lot No.: 302-402926858 Adjust. Gas Exp.: 12/19/2026  
0.300% Dry Gas Lot No.: 302-402755077 Adjust. Gas Exp.: 05/26/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	17:23:31		*TEST PASSED*
Control .04 Test 1 EC	0.040	17:24:05	1011	*TEST PASSED*
Control .04 Test 1 IR	0.040	17:24:05	1011	*TEST PASSED*
Ambient Air Blank	0.000	17:25:12		*TEST PASSED*
Control .04 Test 2 EC	0.041	17:25:24	1011	*TEST PASSED*
Control .04 Test 2 IR	0.040	17:25:24	1011	*TEST PASSED*
Ambient Air Blank	0.000	17:28:07		*TEST PASSED*
Control .08 Test 3 EC	0.078	17:28:42	1011	*TEST PASSED*
Control .08 Test 3 IR	0.080	17:28:42	1011	*TEST PASSED*
Ambient Air Blank	0.000	17:29:57		*TEST PASSED*
Control .08 Test 4 EC	0.080	17:30:09	1012	*TEST PASSED*
Control .08 Test 4 IR	0.081	17:30:09	1012	*TEST PASSED*
Ambient Air Blank	0.000	17:33:31		*TEST PASSED*
Control .16 Test 5 EC	0.156	17:34:09	1011	*TEST PASSED*
Control .16 Test 5 IR	0.159	17:34:09	1011	*TEST PASSED*
Ambient Air Blank	0.000	17:35:30		*TEST PASSED*
Control .16 Test 6 EC	0.160	17:35:45	1011	*TEST PASSED*
Control .16 Test 6 IR	0.160	17:35:45	1011	*TEST PASSED*
Ambient Air Blank	0.000	17:42:14		*TEST PASSED*
Control .30 Test 7 EC	0.300	17:42:49	1012	*TEST PASSED*
Control .30 Test 7 IR	0.305	17:42:49	1012	*TEST PASSED*
Ambient Air Blank	0.000	17:44:18		*TEST PASSED*
Control .30 Test 8 EC	0.308	17:44:31	1011	*TEST PASSED*
Control .30 Test 8 IR	0.308	17:44:31	1011	*TEST PASSED*
Ambient Air Blank	0.000	17:45:10		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Bellay - First Name: David MI: M. Badge No.: 8112

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

 8112

Signed:

Date: 02/26/2026

ID: 50

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 1**  
*Seaside Heights*  
**SERIAL NUMBER: ARMK-0265**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
 Cyl1 Install File No.: 111 Cyl1 Install Date: 07/29/2024 Cyl1 Install No.: 2

**Control Tests (0.100%)**

Installation Inlet: #1 (Upper) Post test active Cyl.: #2 (Lower)  
 Dry Gas Lot No.: 302-402843436 Dry Gas Lot Exp.: 09/08/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	10:17:45		*TEST PASSED*
Control Test 1			1016	*TEST PASSED*
EC Result	0.097	10:18:31		*TEST PASSED*
IR Result	0.100	10:18:31		*TEST PASSED*
Ambient Air Blank	0.000	10:19:43		*TEST PASSED*
Control Test 2			1016	*TEST PASSED*
EC Result	0.100	10:20:07		*TEST PASSED*
IR Result	0.100	10:20:07		*TEST PASSED*
Ambient Air Blank	0.000	10:21:21		*TEST PASSED*
Control Test 3			1016	*TEST PASSED*
EC Result	0.100	10:21:45		*TEST PASSED*
IR Result	0.100	10:21:45		*TEST PASSED*
Ambient Air Blank	0.000	10:22:17		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Waldrop - First Name: Robert MI: W Badge No.: 8256

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*TRC Waldrop # 8256*

Signed:

Date: 07/29/2024

ID: 52

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 2**  
**Seaside Heights**  
**SERIAL NUMBER: ARMK-0265**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
 Cyl2 Install File No.: 211 Cyl2 Install Date: 02/26/2026 Cyl2 Install No.: 2

**Control Tests (0.100%)**

Installation Inlet: #2 (Lower) Post test active Cyl.: #1 (Upper)  
 Dry Gas Lot No.: 302-403034214 Dry Gas Lot Exp.: 05/02/2027

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	17:57:39		*TEST PASSED*
Control Test 1			1012	*TEST PASSED*
EC Result	0.099	17:58:25		*TEST PASSED*
IR Result	0.100	17:58:25		*TEST PASSED*
Ambient Air Blank	0.000	17:59:42		*TEST PASSED*
Control Test 2			1012	*TEST PASSED*
EC Result	0.100	18:00:06		*TEST PASSED*
IR Result	0.101	18:00:06		*TEST PASSED*
Ambient Air Blank	0.000	18:01:27		*TEST PASSED*
Control Test 3			1012	*TEST PASSED*
EC Result	0.101	18:01:51		*TEST PASSED*
IR Result	0.102	18:01:51		*TEST PASSED*
Ambient Air Blank	0.000	18:02:27		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Bellay - First Name: David MI: M. Badge No.: 8112

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*David Bellay 8112*

Signed:

Date: 02/26/2026

ID: 50

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036  
DRAEGER MEDICAL SYSTEMS INC

Sales order: 1123816776  
Date: September 18, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402843436  
ETHANOL IN NITROGEN

Product Expiration: September 08, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	263.3	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS  
TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: September 08, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 170.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036  
**DRAEGER MEDICAL SYSTEMS INC**

Sales order: 1130435101  
 Date: May 28, 2024

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
 ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
 CALGAZ LOT#: 302-403034214  
 ETHANOL IN NITROGEN

Manufactured Date: May 02, 2024  
 Product Expiration: May 02, 2027

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>		
ETHANOL	264.9	(0.102)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND28529	103.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.


Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

APPROVED BY: \_\_\_\_\_

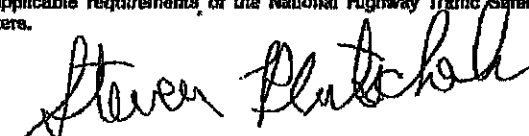

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
 821 Chesapeake Drive, Cambridge, MD 21613-0149  
 Phone: (410) 228-6400 Fax: (410) 228-4251

  
**Dräger****Alcotest 9510****CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:


Serial Number:

10/31/2023ARMK-0265

Dräger, Inc.

BLS IP  

---





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

PHILIP D. MURPHY  
Governor

TAHESHA L. WAY  
Lt. Governor

MATTHEW J. PLATKIN  
Attorney General

COLONEL PATRICK J. CALLAHAN  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

**MANUFACTURER:** Dräger, Inc.

**ANALYSIS DATE:** 06/17/2025

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 25180

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1221 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 03, 2027.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Michael Kennedy*  
Michael Kennedy  
Director  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of June, 2025.

*[Signature]*  
Notary

KAREN E. STAHL  
Notary Public, State of New Jersey  
Comm. # 50110522  
My Commission Expires 8/13/2029



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable



**CALIBRATED** **CERTIFICATE OF CALIBRATION**  
BY TRANSCAT

Customer: DRAEGER INC  
 7288 S EAM HOUSTON PIQWY W  
 STE 100  
 HOUSTON, TX 77066  
 PO Number: SLG430370082



Certificate/SO Number: 5-F8B2G-420-1 Revision 0

Manufacturer: Dräger Safety AG & Co. KGaA  
 Model Number: X-Gal 2000  
 Description: Breath Alcohol Simulator  
 Serial Number: ARPD-0011  
 ID: NONE

As-Founds in Tolerance  
 As-Limits in Tolerance  
 Issue Date: Aug 10, 2025  
 Calibration Date: Aug 11, 2025  
 Due Date: Aug 10, 2026

Calibrated To: Manufacturer Specification  
 Calibration Procedure: 1-AC (036) 9-2

Transcat Calibration Laboratories have been studied and found to comply with ISO/IEC 17025:2017. Approved certificates performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any discrepancies exist are noted as Waiver not covered by the Lab Scope of Accreditation and listed in the notes portion of the certificate. SOC, NDC, RAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual (TQM-QM), the customer Purchase Order and/or Quality Agreement requirements, ISO 60312:16, ANSI/NCSL Z540-1:184 (2020), and ISO 10012:2003 as applicable. Upon specific request, the requirements of ISO 15189:2013, ISO/IEC 17025-1:2005/ISO 17025-2:2005, and ANSI/NCSL Z540-3:2003 (2017) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat determines the suitability of measurement in the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national metrological institutes (NMI) that are affiliated to the OIML (International Organization for Standardization) or accepted Government and/or other physical constants, or by the use of specialized methods, consistent standards or ratio type measurements. Documentation supporting uncertainty information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further determination of traceability.

Uncertainties are reported with a coverage factor k=2, providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TMR of <math>10^{-6}</math> or better (2.4 for mass calibrations), unless otherwise noted. The 1-sigma Uncertainty Ratio (TUR) is calculated in accordance with NIST Generalized MPE-1a. For mass calibrations: Conventional mass tolerances in <math>0.02</math> g/cm<sup>3</sup>.

The results in this report relate only to the items calibrated or tested. Recalibration data is valid in the scope of calibration within the stated uncertainties at the environmental conditions noted. This determination of compliance in the specification is specific to the model/serial number, referenced above based on the tolerance shown. These tolerances are identical to original equipment manufacturers ( OEMs) specified specifications or the client's indicated specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this equipment are detailed in the OEM's operating instructions. This certificate may not be reproduced, stored, or used without the written approval of Transcat. Additional information, if applicable, may be included on separate reports.

Date Received: August 09, 2025  
 Service Level: RP

Certificate Page 1 of 6  
 Issued on December 03, 2025

Customer Number: 1-090111-000  
 DRSG-20-0 (REV 6/22/23) TP00199 4/26/2021

# CALIBRATED CERTIFICATE OF CALIBRATION

BY TRANSOAT

Customer: DRAEGER INC  
 7266 G SAM HOUSTON PIQWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: BUC4305700802



Certificate/SO Number: 8-F8B2G-420-1 Revision 0

As Found/As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	Cal Process Uncertainty (Res: 1)	Measurement Uncertainty (k=2) (2)	Units	TDR
Function Checks									
Bubble Check			P	P	P				
Salt Check			P	P	P				
Temperature Source: Accuracy Test									
Accuracy Test	34.00°C	±(0.02 °C)	33.98	34.02	34.01 °C	1.5e-002	1.5e-002	°C	1.3:1
Temperature Source: Stability Test									
Stability Test	0.00°C	±(0.02 °C)	-0.02	0.02	0.00 °C	1.5e-002	1.5e-002	°C	1.3:1

Find not applicable.

Traceable Standards

Asset#	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
0511476	Acculab Dispenslon	AM1730-12-R	Secondary SPRT	12-Aug-24	31-Aug-26	1122004-1	AP/AL
HP627312	Fluke Standards/Filco	1875	Super Thermometer	15-Jul-24	31-Jan-26	0-611P927312-9-1	AP/AL

The use of the standard is defined as: AP - used for as-found readings, AL - used for as-left readings.

Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
65.80°F (21.00°C)	68.00%	Dowd/11	G	Temperature

Decision Rule

When compliance statements are present, they are reported without deviating in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zone is defined as: greater than the high limit, and/or less than the low limit. Single measurement results in the acceptance zone.

Date Received: August 05, 2025  
 Revision Level: R0

Certificate - Page 2 of 6  
 Registered on December 02, 2025

Customer Number: 1-650311-000  
 OPE-F20 014111 072725 F20U10 452021

# CALIBRATED BY TRANSCAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
7236 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77056  
PO Number: SUC4303700862



Certificate/SO Number: 6-F8B2Q-420-1 Revision 0

are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same parameter, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the previous reading does not represent the system under test. Statements of conformity are binary.

Date Received: August 08, 2025  
Device Label: RA

Certificate - Page 3 of 5  
Revised on December 03, 2025

Customer Number: 1-050111-000  
DPS-420-01AR1 07/27/23 PFC0164 4/0/2021

# CALIBRATED CERTIFICATE OF CALIBRATION

By TRANSOFT

Customer: DRAEGER INC  
 7266 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77066  
 PO Number: SUC4903708052



Certificate/CO Number: 5-F8B2G-420-1 Revision 0

Topic	Description
Accuracy	UUT specifications that establishes expected tolerance and a bias limit (calibration tolerance) over which the instrument is expected to hold those tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (C)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a redaction to the original certificate has been issued
Low / High Limits	Establishes UUT acceptance performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OQA	Out of Acceptance (O)
ODT	Out of Tolerance (T)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

Date Issued: August 06, 2005  
 Service Level: RS

Certificate - Page 4 of 5  
 Replaced on December 03, 2005

Customer Number: 1-659111-000  
 CP9-F8B-01A(1) 02/27/03 F8B100 4/0/0081

**CALIBRATED** CERTIFICATE OF CALIBRATION  
BY TRANSCAT

Customer: DRAEGER INC  
 7266 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77065  
 PO Number: SLIC4303700082



Certificate/SO Number: 5-F8B2G-420-1 Revision 0

Calibrated At:  
 18115 Park Row  
 Houston, TX 77064

Facility Responsible:  
 18115 Park Row  
 Houston, TX 77064  
 800-828-1470

Calibrated By:  
 Electronically Signed By:  
 Jose Martinez

Revised By:  
 Electronically Signed By:  
 David Weigle Inc

Unit Barcode:



Jose Martinez Aug 16, 2025  
 Definition Termination 14:58:01 -04:00

Jose Bellan Aug 15, 2025  
 Lpb Mreupm 10:32:45 -04:00


Date Received: August 06, 2025  
 Barcode Label: R9

Certificate - Page 5 of 5  
 Reprinted on December 03, 2025

Customer Number: 1-060711-000  
 OPS #20 0141011 072229 FP00100407021

# CALIBRATED BY TRANSCAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77065  
PO Number: SUC4303700862

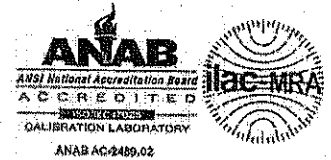

Certificate/SO Number: 5-F8B2G-40-1 Revision 0

Manufacturer: Mensor Corp  
Model Number: CPG2300  
Description: Portable Barometer  
Serial Number: 41001275  
ID: NONE

As-Found: Out Of Tolerance  
As-Left: In Tolerance

Issue Date: Aug 25, 2025  
Calibration Date: Aug 23, 2025  
Due Date: Aug 23, 2026

Calibrated To: Manufacturer Specification  
Calibration Procedure: 1-AC107289-0

Transcat Calibration Laboratories have been audited and found in compliance with ISO 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. GSC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/NCCL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS 16949:2009, 10CFR21, 10CFR40 App. B, ASME NQA-1:2012, and ANSI/NCCL Z540.3-2008 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the OIML Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCCL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Reported calibration data is valid at the time of calibration with the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturer's (OEM's) warranted specifications or the client's requested specifications. Any number of factors may cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate reports.

Notes:

Unit received out of tolerance. Adjustments were made to meet customer specs.

The COI readings were verified.

Date Received: August 08, 2025  
Service Level: R2


Certificate - Page 1 of 6  
Reprinted on August 27, 2025

Customer Number: 1-858111-000  
DPB-F20-014R31 07/27/23 FP00109 4/8/2021

**CALIBRATED**  
BY TRANSCIT

**CERTIFICATE OF CALIBRATION**

Customer: DRAEGER INC  
7236 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77065  
PO Number: SUC4303700862

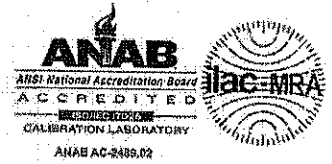

Certificate/SO Number: 5-F8B2G-40-1 Revision 0

As Found Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found	O D Y	Cal Process Uncertainty (k=2; σ)	Measurement Uncertainty (k=2; σ)	Units	TUR
Pressure Measure: 552 to 1172 mbars Range										
	550.07mbars	±(0.015% FS)	549.9	550.3	549.7 mbars	*	1.0e-002	6.1e-002	mbars	19.1:1
	610.01mbars	±(0.015% FS)	609.5	610.2	609.7 mbars	*	1.2e-002	5.9e-002	mbars	17.3:1
	680.39mbars	±(0.015% FS)	680.2	680.6	680.0 mbars	*	1.3e-002	5.9e-002	mbars	16.5:1
	734.28mbars	±(0.015% FS)	734.1	734.5	733.8 mbars	*	1.4e-002	5.9e-002	mbars	14.3:1
	804.64mbars	±(0.015% FS)	804.4	804.8	804.3 mbars	*	1.6e-002	6.0e-002	mbars	13.1:1
	864.92mbars	±(0.015% FS)	864.7	865.1	864.9 mbars	*	1.6e-002	6.0e-002	mbars	12.2:1
	924.92mbars	±(0.015% FS)	924.7	925.1	924.6 mbars	*	1.8e-002	6.0e-002	mbars	11.4:1
	985.22mbars	±(0.015% FS)	985.0	985.4	984.9 mbars	*	1.9e-002	6.1e-002	mbars	10.7:1
	1043.86mbars	±(0.015% FS)	1043.7	1044.1	1043.5 mbars	*	2.0e-002	6.1e-002	mbars	10.1:1
	1114.30mbars	±(0.015% FS)	1114.0	1114.4	1113.8 mbars	*	2.1e-002	6.1e-002	mbars	9.4:1
	1174.59mbars	±(0.015% FS)	1174.4	1174.8	1174.2 mbars	*	2.2e-002	6.2e-002	mbars	9.0:1
	924.92mbars	±(0.015% FS)	924.7	925.1	924.6 mbars	*	1.8e-002	6.0e-002	mbars	11.4:1
	864.92mbars	±(0.015% FS)	864.7	865.1	864.6 mbars	*	1.6e-002	6.0e-002	mbars	12.2:1
	804.64mbars	±(0.015% FS)	804.4	804.8	804.3 mbars	*	1.5e-002	6.0e-002	mbars	13.1:1


Date Received: August 08, 2025  
Service Level: R9

Certificate - Page 2 of 6  
Reprinted on August 27, 2025

Customer Number: 1-859111-000  
DPS-F20-014R11 07/27/23 FP001R9 4/9/2021

# CALIBRATED BY TRANSCOT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
 7258 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: SUC4303700862

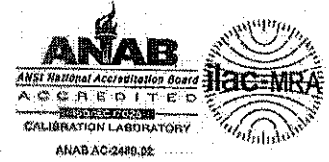

Certificate/SO Number: 5-F8B2G-40-1 Revision 0

As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Left	Cal Process Uncertainty (k=2; ±)	Measurement Uncertainty (k=2; ±)	Units	TUR
Pressure Measure: 552 to 1172 mbara Range									
	550.07mbara	±(0.015% FS)	549.9	550.3	550.1 mbara	1.0e-002	6.1e-002	mbara	19.1:1
	610.01mbara	±(0.015% FS)	609.8	610.2	610.1 mbara	1.2e-002	6.9e-002	mbara	17.3:1
	680.37mbara	±(0.015% FS)	680.2	680.5	680.4 mbara	1.3e-002	6.9e-002	mbara	15.9:1
	734.27mbara	±(0.015% FS)	734.1	734.6	734.3 mbara	1.4e-002	6.9e-002	mbara	14.3:1
	804.64mbara	±(0.015% FS)	804.4	804.8	804.7 mbara	1.5e-002	6.0e-002	mbara	13.1:1
	864.91mbara	±(0.015% FS)	864.7	865.1	865.0 mbara	1.6e-002	6.0e-002	mbara	12.2:1
	924.91mbara	±(0.015% FS)	924.7	925.1	925.0 mbara	1.6e-002	6.0e-002	mbara	11.4:1
	985.21mbara	±(0.015% FS)	985.0	985.4	985.3 mbara	1.6e-002	6.1e-002	mbara	10.7:1
	1043.64mbara	±(0.015% FS)	1043.5	1044.0	1043.9 mbara	2.0e-002	6.1e-002	mbara	10.1:1
	1114.19mbara	±(0.015% FS)	1114.0	1114.4	1114.2 mbara	2.1e-002	6.1e-002	mbara	9.4:1
	1174.65mbara	±(0.015% FS)	1174.4	1174.8	1174.6 mbara	2.2e-002	6.2e-002	mbara	9.0:1
	924.91mbara	±(0.015% FS)	924.7	925.1	925.0 mbara	1.6e-002	6.0e-002	mbara	11.4:1
	864.91mbara	±(0.015% FS)	864.7	865.1	865.0 mbara	1.6e-002	6.0e-002	mbara	12.2:1
	804.63mbara	±(0.015% FS)	804.4	804.8	804.7 mbara	1.5e-002	6.0e-002	mbara	13.1:1

Field not applicable.

Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
DW11BA	Fluke/DH Instruments	PG7601	Piston Gauge	31-Jul-25	31-Jul-26	5-8DW11BA-20-1	AF/AL
DW11CA	Fluke/DH Instruments	MS-AMH-36	AMH Mass Set	5-Jun-25	30-Sep-25	5-8DW11CA-40-1	AF/AL
DW11LOW	Fluke/DH Instruments	PC-7100/7800-10-TC	Gas Piston-Cylinder Module	8-Apr-22	30-Apr-27	5-8DW11LOW-3-1	AF/AL
DW11MASS	Fluke/DH Instruments	MS-AMH-36	AMH Mass Set	5-Mar-25	31-Mar-26	5-8DW11MASS-12-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

Date Received: August 08, 2025  
 Service Level: R3

Certificate - Page 3 of 6  
 Reprinted on August 27, 2025

Customer Number: 1-659111-000  
 DPS-F20-014R11 07/27/23 FPC01R3 4/9/2021

**CALIBRATED**  
BY TRANSOIT

# CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77065  
PO Number: SUC4303700882



Certificate/SO Number: 5-F8B2G-40-1 Revision 0

### Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
73.10°F /22.83°C	43.00%	DewK9	B	GP Pressure

### Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.


Date Received: August 09, 2025  
Service Level: R9

Certificate - Page 4 of 6  
Reprinted on August 27, 2025

Customer Number: 1-858111-000  
OPS-F26-014R11 07/27/23 FP001R0 4/9/2021

# CALIBRATED BY TRANSCOT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77065  
 PO Number: SUC4303700662

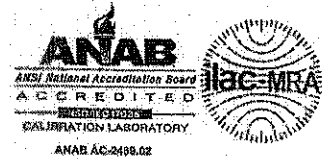

Certificate/SO Number: 5-F8B2G-40-1 Revision 0

## Legend

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (K)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
COA	Out of Acceptance (B)
COT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

Date Received: August 08, 2025  
 Service Level: RS

Certificate - Page 5 of 6  
 Reprinted on August 27, 2025

Customer Number: 1-659111-000  
 OPS-F20-014R11 07/27/25 FP001RS 4/9/2021

# CALIBRATED BY TRANSCAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
7266 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77065  
PO Number: SUC4302700862



Certificate/SO Number: 5-F8B2G-40-1 Revision 0

Calibrated At:  
16115 Park Row  
Houston, TX 77064

Facility Responsible:  
16115 Park Row  
Houston, TX 77064  
800-828-1470

Calibrated By:

Electronically Signed By:  
Alex Spilker

Reviewed By:

Electronically Signed By:  
Grafton Walker for

Unit Barcode:   
09008428043

Alex Spilker Aug 23, 2025  
Calibration Technician 20:24:59 -04:00

Josh Soltsev Aug 25, 2025  
Lab Manager 06:31:52 -04:00

Date Received: August 08, 2025  
Service Level: R9

Certificate - Page 5 of 6  
Reprinted on August 27, 2025

Customer Number: 1-659111-000  
OPS-F20-014R11 072723 FP001R9 4/9/2021

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DEPT OF LAW AND PUBLIC SAETY

Sales order: 1120654933  
Date: May 30, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402755160  
ETHANOL IN NITROGEN

Product Expiration: May 24, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	261.6	(0.100)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS.

#### TRACEABILITY

##### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 24, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DEPT OF LAW AND PUBLIC SAFETY

Sales order: 1120656707

Date: May 30, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater:

CALGAZ LOT#: 302-402730318

ETHANOL IN NITROGEN

Product Expiration: April 27, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	104.2PPM	(0.040)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	(BrAC)
ETHANOL	107.8	(0.041)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS:

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company, using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (GIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: April 27, 2023

APPROVED BY:

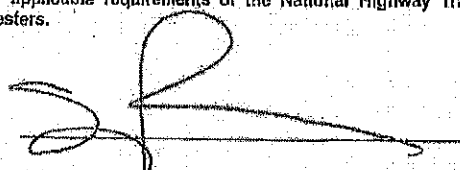

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DEPT OF LAW AND PUBLIC SAFETY

Sales order: 1120656618

Date: May 25, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402732434  
ETHANOL IN NITROGEN

Product Expiration: April 28, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	208.4PPM	(0.080)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	210.4	(0.081)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: April 28, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC.

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401040NJ  
**DRAEGER MEDICAL SYSTEMS INC**

Sales order: 1128582210  
 Date: March 18, 2024

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
 ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
 CALGAZ LOT#: 302-402926858  
 ETHANOL IN NITROGEN

Product Expiration: December 19, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	416.8PPM	(0.160)
NITROGEN	BAL	
<hr/>		
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	419.3	(0.161)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**


Preparation:  
 Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.  
 Traceable certificate numbers 3445312 and 3398673.

Analytical:  
 Analytical Instruments Calibrated Using NMI Traceable Standards.  
 Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
 CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: December 19, 2023

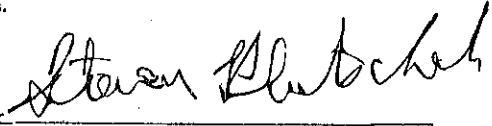APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
 821 Chesapeake Drive, Cambridge, MD 21613-0149  
 Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DEPT OF LAW AND PUBLIC SAFETY

Sales order: 1120654720

Date: May 30, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-402755077

ETHANOL IN NITROGEN

Product Expiration: May 26, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	781.6PPM	(0.300)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	794.4	(0.305)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 26, 2023

APPROVED BY:



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251



DEPARTMENT OF  
**Water and Public Safety**  
*This is to certify that*

**Robert W. Waldrop**

**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1946 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF March

TWO THOUSAND AND Twenty Four

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 283B (Rev. 10/22)

DEPARTMENT OF  
**Water and Public Safety**  
*This is to certify that*

**Robert W. Waldrop**

**New Jersey State Police**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1946 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF April

TWO THOUSAND AND Twenty Three

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 283B (Rev. 10/22)