


STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENTATION SERVICE REPORT

1. Department: Seaside Heights Police Dept. 116 Sherman Ave Seaside Heights, NJ 08751	2. Contact: Sgt. Roemmele	4. Date: 9/23/2013
	3. Phone Number: (732) 793-1800	5. County: Ocean
6. Alcotest Instrument Serial Number: ARWJ-0018	7. Simulator Component Serial Number: N/A	8. Temperature Probe Component Serial Number: N/A

9. Reason for Service:
Returned from Draeger.

10. Comments:
Instrument was put back into service and a Calibration was performed on same with positive results.

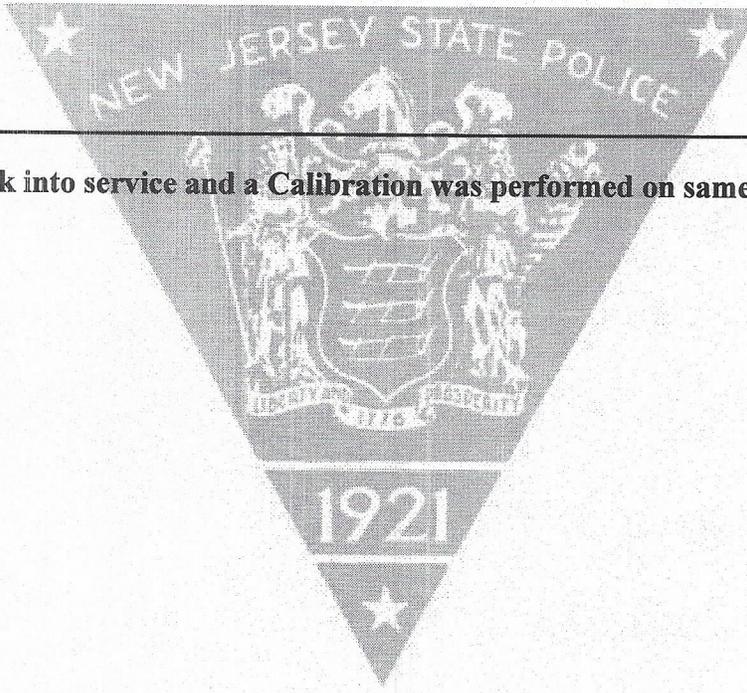

11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.

12. The above Instrument/Component is placed out of service pending further evaluation.

13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."

Sgt. Marc Dennis #5925

Name & Badge Number (Print)

Sgt. Marc Dennis

Signature

9/23/13

Date

RETURN AND REPAIR FORM



Customer Information

B: _____ S: _____

Company Name: Seaside Heights P.D., Seaside Heights, NJ

Date Received: 09/12/13

Date given to service: 09/12/13

Carrier: FedEx UPS USPS Shipping Method: GRD 3DAY 2DAY
 NDA-PRI NDA-STD

Product: 6510 6810
 7110 8610
 7510 DT5000
 7410 Upper-half 9510
 7410 Whole

Serial Number: AR WJ-0018

Printer Serial#: AR

Sim Serial#: DD

Probe Serial#: DD

Warranty Expires: January 2014

Description: A B Plus Demo Screener Trade In

Accessories

110V A/C Adapter Regulator Printer Ribbon Printer Paper
 Mouthpieces 9510 Stylus 9510 Top Cover Carrying Case
 Dry Gas Other (please specify) _____

Repair Information:

Test#: _____

Part Number	Description	Qty	Total Cost
MP Cal 71	Calibration	1	NC/W
MP Labor	Labor	8	NC/W
8315075	Alcotest 7110 Motherboard	1	NC/W

Repair Notes: Replaced defective motherboard for external printing issues.

CAL W/QC AND OPS CHECK

Service Technician: BC

Date: 09/13/13

Packing Slip

Customer no Order No Order date
 150060725 10651512 09/17/2013


Packing slip no. Ship date
 80803661 09/17/2013

Please reference on inquiries

ship to

150060729
 BOROUGH OF SEASIDE HEIGHTS POLICE
 ATTN: CHIEF THOMAS J. BOYD
 OCEAN COUNTY
 116 SHERMAN AVENUE
 SEASIDE HEIGHTS, NJ 08751
 USA

bill to

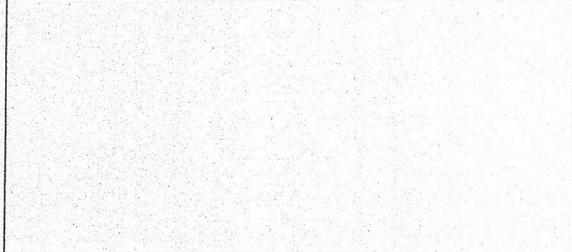

Your Purchase Order Number

7110: ARWJ-0018
 Any questions? Please contact:
 MARA HERRERA

Your sales person

Don Pouliot
 Phone: 973-398-3228

Customer
 BOROUGH OF SEASIDE HEIGHTS
 MUNICIPAL BUILDING
 OCEAN COUNTY
 901 BLVD-PO BOX 38
 SEASIDE HEIGHTS, NJ 08751
 USA

Delivery terms

FA
 FREIGHT ALLOWED

Page 1 / 2

Item#	sh. Quant.	Part no. Description			
		Ship via: Fed Ex Saver			
		NOTE: All claims for shortages/defects must be reported within 10 Business days after receipt of order. All returns must have our RMA# clearly marked on the box. Please call Customer Service at 866-385-5900.			
		7110: ARWJ-0018			
0010	1 EA	MPCAL71 CALIBRATION CHARGE - 7110/9510 Ordered / Back ordered : 0 / 0 EA			
0020	1 EA	8315075 PCB,ALCOTEST 7110 MKII US VERSION Ordered / Back ordered : 0 / 0 EA			

Draeger Safety Diagnostics Inc.
 Accounting Address:
 101 Technology Drive
 Pittsburgh, PA 15275
 Tel: (412) 788-5537
 Fax: (412) 788-5598

Remit Wire Transfers To:
 Citizens Bank
 Acct. # 6209426615
 Acct. Name: Draeger Safety Diagnostics Inc.
 Transit Number: 036076150
 Federal ID Number: 84-1600159

REMIT TO:
 Draeger Safety Diagnostics Inc.
 P.O. Box 200337
 Pittsburgh, PA 15251-0337

Packing Slip

Customer no Order No Order date
150060725 10651512 09/17/2013

Packing slip no. **Ship date**
80803661 09/17/2013

Please reference on inquiries

Page 2 / 2

Item#	sh. Quant.	Part no. Description			
0030	8 H	MPLABOR LABOR CHARGE Ordered / Back ordered : 0 / 0 H			

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENTATION SERVICE REPORT

1. Department: Seaside Heights Police Dept. 116 Sherman Ave Seaside Heights, NJ 08751	2. Contact: Sgt. Roemmele	4. Date: 9/5/2013
	3. Phone Number: (732) 793-1800	5. County: Ocean
6. Alcotest Instrument Serial Number: ARWJ-0018	7. Simulator Component Serial Number: N/A	8. Temperature Probe Component Serial Number: N/A

9. Reason for Service:
I was contacted and advised that the instrument was experiencing printing issues. They also advised that they obtained a new printer and attached same, however they were still having same issues. I checked the attachments on the printer and also confirmed it was a compatible one. I conducted a solution change and the instrument read data stored and printing and it returned to the ready mode, however nothing printed. I utilized the print functions and it displayed printing and went back to ready mode, but still nothing printed. I then utilized my black key probe to check the memory and it indicated 0.0 %

10. Comments:
Operational condition of the instrument was assessed by reviewing the performance history of the instrument along with aforementioned checks and it was determined that the instrument was experiencing a problem printing the data which is possibly related to the memory of the 7110. Instrument was placed out of service and returned to Draeger Safety Diagnostics for evaluation.

- 11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
- 12. The above Instrument/Component is placed out of service pending further evaluation.
- 13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."

Sgt. Marc Dennis #5925

Name & Badge Number (Print)

Sgt. M. Dennis

Signature

9/5/13

Date