

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01108 Calib. Date: 02/24/2015 Calib. No.: 00025
Certification File No.: 01109 Cert. Date: 02/24/2015 Cert. No.: 00018
Linearity File No.: 01110 Lin. Date: 02/24/2015 Lin. No.: 00018
Solution File No.: 01138 Soln. Date: 05/22/2015 Soln. No.: 00206
Sequential File No.: 01138 File Date: 05/22/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0440
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 0751

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:10D		
Control 1 EC	0.100%	05:11D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	05:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:11D		
Control 2 EC	0.100%	05:12D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:13D		
Control 3 EC	0.100%	05:13D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	05:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: _____

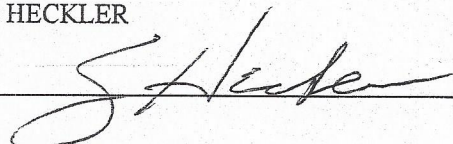

Badge No.: 120

Date: 05/22/2015