

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01108	Calib. Date: 02/24/2015
Certification File No.:	01109	Cert. No.: 00025
Linearity File No.:	01110	Cert. Date: 02/24/2015
Solution File No.:	01158	Lin. No.: 00018
Sequential File No.:	01158	Soln. No.: 00207
		File Date: 06/21/2015

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWL S3-0440
Control Solution %: 0.100%		Expires: 06/20/2016
Solution Control Lot: 14F130		Bottle No.: 0774

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:43D		
Control 1 EC	0.102%	08:44D	34.0°C	AMBIENT AIR CHECK ERR
Control 1 IR	-.---%	08:44D	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	-.---%	08:44D		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ROEMMELE

First Name: RICHARD

MI: R

Signature: _____

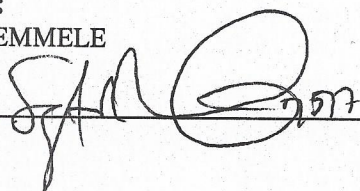

Badge No.: 97517

Date: 06/21/2015