

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	01108	Calib. Date:	02/24/2015
Certification File No.:	01109	Cert. No.:	00025
Linearity File No.:	01110	Lin. Date:	02/24/2015
Solution File No.:	01178	Lin. No.:	00018
Sequential File No.:	01178	Soln. Date:	07/24/2015
		Soln. No.:	00211
		File Date:	07/24/2015

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWL S3-0440
Control Solution %:	0.100%			Expires:	06/20/2016
Solution Control Lot:	14F130			Bottle No.:	0771

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:49D		
Control 1 EC	0.098%	23:50D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	23:50D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:50D		
Control 2 EC	0.098%	23:51D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	23:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:52D		
Control 3 EC	0.098%	23:52D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	23:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: _____

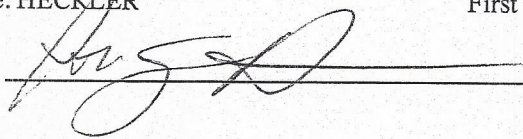

Badge No.: 120

Date: 07/24/2015