

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	01187	Calib. Date:	08/03/2015
Certification File No.:	01188	Cert. Date:	08/03/2015
Linearity File No.:	01189	Lin. Date:	08/03/2015
Solution File No.:	01199	Soln. Date:	08/16/2015
Sequential File No.:	01199	File Date:	08/16/2015

Calib. No.:	00026
Cert. No.:	00019
Lin. No.:	00019
Soln. No.:	00215

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWL S3-0440
Control Solution %:	0.100%			Expires:	06/20/2016
Solution Control Lot:	14F130			Bottle No.:	0763

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:07D		
Control 1 EC	0.097%	03:08D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:08D		
Control 2 EC	0.098%	03:09D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:10D		
Control 3 EC	0.097%	03:10D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	03:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: \_\_\_\_\_

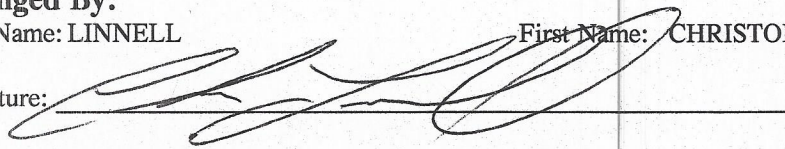

Badge No.: 128

Date: 08/16/2015