

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWJ-0018  
**Location:** SEASIDE HEIGHTS POLICE  
**Calibration File No.:** 01187 **Calib. Date:** 08/03/2015 **Calib. No.:** 00026  
**Certification File No.:** 01188 **Cert. Date:** 08/03/2015 **Cert. No.:** 00019  
**Linearity File No.:** 01189 **Lin. Date:** 08/03/2015 **Lin. No.:** 00019  
**Solution File No.:** 01219 **Soln. Date:** 09/03/2015 **Soln. No.:** 00219  
**Sequential File No.:** 01219 **File Date:** 09/03/2015

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDWL S3-0440  
**Control Solution %:** 0.100% **Expires:** 06/20/2016  
**Solution Control Lot:** 14F130 **Bottle No.:** 0766

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:47D		
Control 1 EC	0.098%	17:48D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	17:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:48D		
Control 2 EC	0.097%	17:49D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	17:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:50D		
Control 3 EC	0.097%	17:50D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:50D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:51D		

All tests within acceptable tolerance.

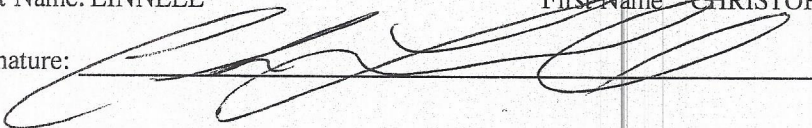
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 09/03/2015