

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01261	Calib. Date: 03/01/2016
Certification File No.:	01262	Calib. No.: 00029
Linearity File No.:	01263	Cert. Date: 03/01/2016
Solution File No.:	01301	Cert. No.: 00021
Sequential File No.:	01301	Lin. Date: 03/01/2016
		Lin. No.: 00021
		Soln. Date: 05/14/2016
		Soln. No.: 00232
		File Date: 05/14/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWL S3-0441
Solution Control Lot:	15F139	Expires: 06/13/2017
		Bottle No.: 0722

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:54D		
Control 1 EC	0.095%	16:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.095%	16:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:56D		
Control 2 EC	0.094%	16:56D	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.094%	16:56D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	16:57D		
Control 3 EC	0.094%	16:58D	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.093%	16:58D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	16:58D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: _____

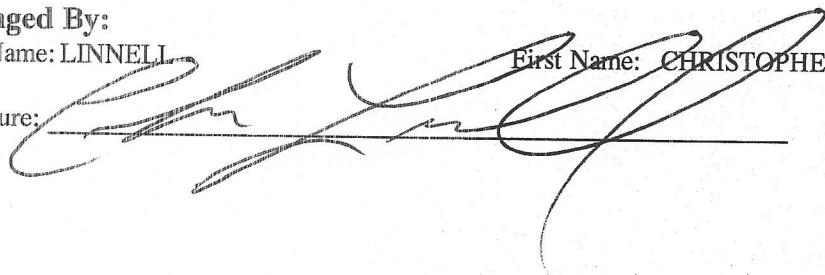

Badge No.: 128

Date: 05/14/2016