

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
<b>Location:</b>	SEASIDE HEIGHTS POLICE	
<b>Calibration File No.:</b>	01261	<b>Calib. Date:</b> 03/01/2016
<b>Certification File No.:</b>	01262	<b>Calib. No.:</b> 00029
<b>Linearity File No.:</b>	01263	<b>Cert. No.:</b> 00021
<b>Solution File No.:</b>	01302	<b>Lin. No.:</b> 00021
<b>Sequential File No.:</b>	01302	<b>Soln. No.:</b> 00233
		<b>File Date:</b> 05/14/2016
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b> CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b> DDWL S3-0441
<b>Solution Control Lot:</b>	15F139	<b>Expires:</b> 06/13/2017
		<b>Bottle No.:</b> 0725

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:26D		
Control 1 EC	0.096%	22:27D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	22:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:28D		
Control 2 EC	0.095%	22:29D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	22:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:29D		
Control 3 EC	0.095%	22:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.095%	22:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: ROEMMELE

First Name: RICHARD

MI: R

Signature: \_\_\_\_\_

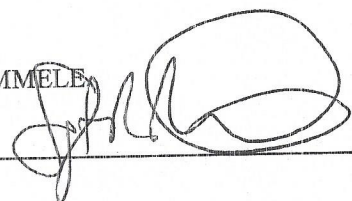

Badge No.: 97517

Date: 05/14/2016