

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01348 Calib. Date: 10/28/2016 Calib. No.: 00032
Certification File No.: 01349 Cert. Date: 10/28/2016 Cert. No.: 00023
Linearity File No.: 01350 Lin. Date: 10/28/2016 Lin. No.: 00023
Solution File No.: 01369 Soln. Date: 12/17/2016 Soln. No.: 00241
Sequential File No.: 01369 File Date: 12/17/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0440
Control Solution %: 0.100% Expires: 05/17/2018
Solution Control Lot: 201605D Bottle No.: 0240

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 23:53S | | |
| Control 1 EC | 0.097% | 23:54S | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.097% | 23:54S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:55S | | |
| Control 2 EC | 0.097% | 23:55S | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.097% | 23:55S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:56S | | |
| Control 3 EC | 0.096% | 23:57S | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.097% | 23:57S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:57S | | |

All tests within acceptable tolerance.

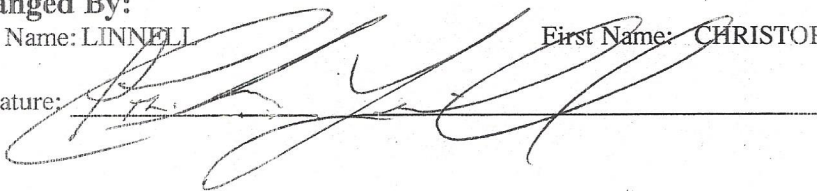
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELI

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 12/17/2016