

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01348	Calib. Date: 10/28/2016
Certification File No.:	01349	Calib. No.: 00032
Linearity File No.:	01350	Cert. Date: 10/28/2016
Solution File No.:	01405	Cert. No.: 00023
Sequential File No.:	01405	Lin. Date: 10/28/2016
		Lin. No.: 00023
		Soln. Date: 03/11/2017
		Soln. No.: 00246
		File Date: 03/11/2017

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWL S3-0440
Control Solution %: 0.100%		Expires: 06/07/2018
Solution Control Lot: 16140		Bottle No.: 0104

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:53S		
Control 1 EC	0.096%	21:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	21:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:55S		
Control 2 EC	0.096%	21:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	21:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:56S		
Control 3 EC	0.096%	21:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	21:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: \_\_\_\_\_

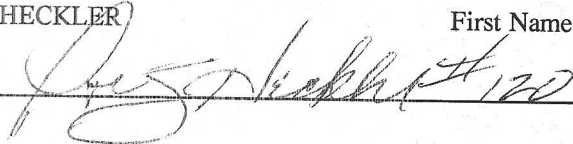

Badge No.: 120

Date: 03/11/2017