

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	01427	Calib. Date:	04/21/2017
Certification File No.:	01428	Cert. Date:	04/21/2017
Linearity File No.:	01429	Lin. Date:	04/21/2017
Solution File No.:	01441	Soln. Date:	05/14/2017
Sequential File No.:	01441	File Date:	05/14/2017

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWL S3-0441
Control Solution %:	0.100%			Expires:	12/02/2018
Solution Control Lot:	16390			Bottle No.:	1052

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:23D		
Control 1 EC	0.098%	19:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	19:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:24D		
Control 2 EC	0.095%	19:25D	34.0°C	AMBIENT AIR CHECK ERR
Control 2 IR	-.---%	19:25D	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	-.---%	19:26D		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature:

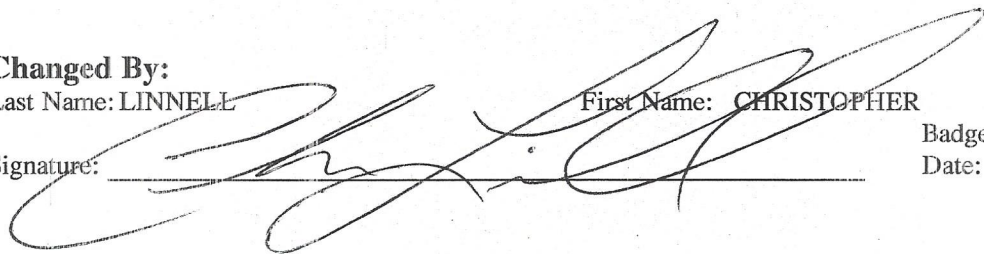

Badge No.: 128

Date: 05/14/2017