

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01427	Calib. Date: 04/21/2017
Certification File No.:	01428	Calib. No.: 00033
Linearity File No.:	01429	Cert. Date: 04/21/2017
Solution File No.:	01468	Cert. No.: 00024
Sequential File No.:	01468	Lin. Date: 04/21/2017
		Lin. No.: 00024
		Soln. Date: 06/10/2017
		Soln. No.: 00255
		File Date: 06/10/2017

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWL S3-0441
Control Solution %: 0.100%		Expires: 12/02/2018
Solution Control Lot: 16390		Bottle No.: 1202

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:42D		
Control 1 EC	0.097%	20:42D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	20:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:43D		
Control 2 EC	0.096%	20:44D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	20:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:45D		
Control 3 EC	0.096%	20:45D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	20:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:46D		

All tests within acceptable tolerance.

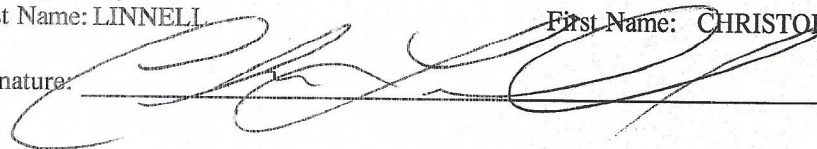
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 06/10/2017