

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01427 Calib. Date: 04/21/2017 Calib. No.: 00033
Certification File No.: 01428 Cert. Date: 04/21/2017 Cert. No.: 00024
Linearity File No.: 01429 Lin. Date: 04/21/2017 Lin. No.: 00024
Solution File No.: 01511 Soln. Date: 08/26/2017 Soln. No.: 00259
Sequential File No.: 01511 File Date: 08/26/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0441
Control Solution %: 0.100% Expires: 12/02/2018
Solution Control Lot: 16390 Bottle No.: 1047

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:17D		
Control 1 EC	0.098%	05:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:19D		
Control 2 EC	0.098%	05:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:20D		
Control 3 EC	0.098%	05:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	05:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:21D		

All tests within acceptable tolerance.

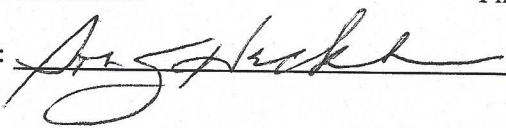
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: 

Badge No.: 120

Date: 08/26/2017