

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01583 Calib. Date: 02/16/2018 Calib. No.: 00035
Certification File No.: 01584 Cert. Date: 02/16/2018 Cert. No.: 00026
Linearity File No.: 01585 Lin. Date: 02/16/2018 Lin. No.: 00026
Solution File No.: 01597 Soln. Date: 03/10/2018 Soln. No.: 00274
Sequential File No.: 01597 File Date: 03/10/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0440
Control Solution %: 0.100% Expires: 12/11/2019
Solution Control Lot: 17420 Bottle No.: 0253

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:59S		
Control 1 EC	0.095%	00:00S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	00:00S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:01S		
Control 2 EC	0.096%	00:01S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	00:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:02S		
Control 3 EC	0.096%	00:03S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:03S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: _____

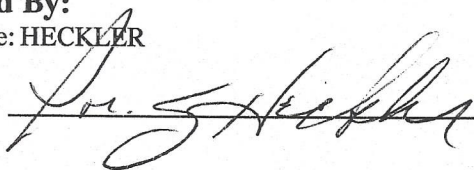

Badge No.: 120

Date: 03/11/2018