

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01583	Calib. Date: 02/16/2018
Certification File No.:	01584	Calib. No.: 00035
Linearity File No.:	01585	Cert. Date: 02/16/2018
Solution File No.:	01619	Cert. No.: 00026
Sequential File No.:	01619	Lin. Date: 02/16/2018
		Lin. No.: 00026
		Soln. Date: 06/09/2018
		Soln. No.: 00277
		File Date: 06/09/2018

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWL S3-0440
Control Solution %: 0.100%		Expires: 12/11/2019
Solution Control Lot: 17420		Bottle No.: 0153

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:05D		
Control 1 EC	-.---%	20:06D	26.1°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	20:06D	26.1°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: \_\_\_\_\_

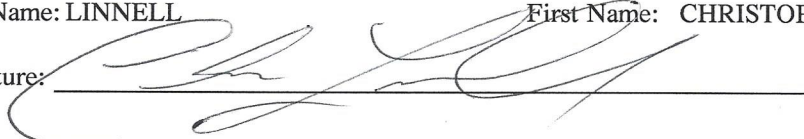

Badge No.: 128

Date: 06/09/2018