

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWJ-0018  
Location: SEASIDE HEIGHTS POLICE  
Calibration File No.: 01644 Calib. Date: 07/24/2018 Calib. No.: 00036  
Certification File No.: 01645 Cert. Date: 07/24/2018 Cert. No.: 00027  
Linearity File No.: 01646 Lin. Date: 07/24/2018 Lin. No.: 00027  
Solution File No.: 01664 Soln. Date: 09/23/2018 Soln. No.: 00282  
Sequential File No.: 01664 File Date: 09/23/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0441  
Control Solution %: 0.100% Expires: 12/11/2019  
Solution Control Lot: 17420 Bottle No.: 0431

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 18:37D |                |                     |
| Control 1 EC      | 0.100% | 18:38D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.100% | 18:38D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 18:38D |                |                     |
| Control 2 EC      | 0.099% | 18:39D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.100% | 18:39D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 18:40D |                |                     |
| Control 3 EC      | 0.099% | 18:40D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.100% | 18:40D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 18:41D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: ROEMMELE

First Name: RICHARD

MI: R

Signature: \_\_\_\_\_

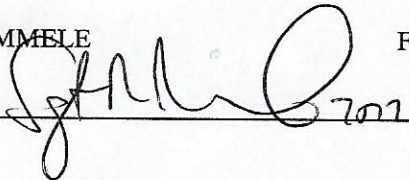

Badge No.: 7517

Date: 09/23/2018