

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01644 Calib. Date: 07/24/2018 Calib. No.: 00036
Certification File No.: 01645 Cert. Date: 07/24/2018 Cert. No.: 00027
Linearity File No.: 01646 Lin. Date: 07/24/2018 Lin. No.: 00027
Solution File No.: 01665 Soln. Date: 09/28/2018 Soln. No.: 00283
Sequential File No.: 01665 File Date: 09/28/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0441
Control Solution %: 0.100% Expires: 12/11/2019
Solution Control Lot: 17420 Bottle No.: 0140

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:29D		
Control 1 EC	0.100%	18:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:30D		
Control 2 EC	0.099%	18:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	18:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:31D		
Control 3 EC	0.099%	18:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	18:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:33D		

All tests within acceptable tolerance.

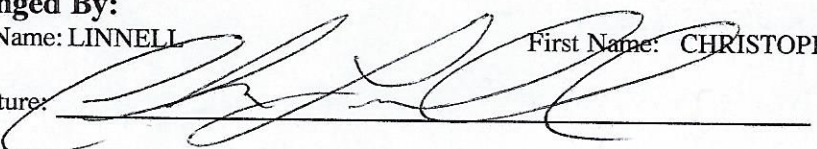
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 09/28/2018