

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	01644	Calib. Date:	07/24/2018
Certification File No.:	01645	Cert. Date:	07/24/2018
Linearity File No.:	01646	Lin. Date:	07/24/2018
Solution File No.:	01677	Soln. Date:	11/22/2018
Sequential File No.:	01677	File Date:	11/22/2018

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWL S3-0441
Control Solution %:	0.100%			Expires:	12/11/2019
Solution Control Lot:	17420			Bottle No.:	0305

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:17S		
Control 1 EC	0.098%	23:17S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	23:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:18S		
Control 2 EC	0.096%	23:19S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	23:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:19S		
Control 3 EC	0.097%	23:20S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	23:20S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: HECKLER

First Name: SHAWN

MI: M

Signature: \_\_\_\_\_

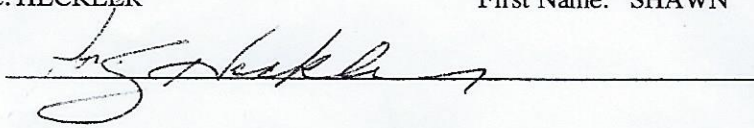

Badge No.: 120

Date: 11/22/2018