

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWJ-0018  
Location: SEASIDE HEIGHTS POLICE  
Calibration File No.: 01644 Calib. Date: 07/24/2018 Calib. No.: 00036  
Certification File No.: 01645 Cert. Date: 07/24/2018 Cert. No.: 00027  
Linearity File No.: 01646 Lin. Date: 07/24/2018 Lin. No.: 00027  
Solution File No.: 01683 Soln. Date: 12/28/2018 Soln. No.: 00286  
Sequential File No.: 01683 File Date: 12/28/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0441  
Control Solution %: 0.100% Expires: 12/11/2019  
Solution Control Lot: 17420 Bottle No.: 0364

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:46S		
Control 1 EC	0.099%	14:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:47S		
Control 2 EC	0.098%	14:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:48S		
Control 3 EC	0.098%	14:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:50S		

All tests within acceptable tolerance.

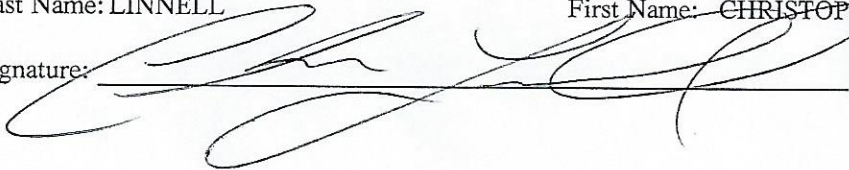
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 12/28/2018