

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01739	Calib. Date: 06/21/2019
Certification File No.:	01740	Calib. No.: 00039
Linearity File No.:	01741	Cert. Date: 06/21/2019
Solution File No.:	01756	Cert. No.: 00030
Sequential File No.:	01756	Lin. Date: 06/21/2019
		Lin. No.: 00030
		Soln. Date: 08/04/2019
		Soln. No.: 00296
		File Date: 08/04/2019

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWL S3-0441
Control Solution %:	0.100%		Expires: 01/08/2021
Solution Control Lot:	19020		Bottle No.: 1435

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:49D		
Control 1 EC	0.099%	16:49D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	16:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:50D		
Control 2 EC	0.099%	16:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:51D		
Control 3 EC	0.098%	16:52D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature:

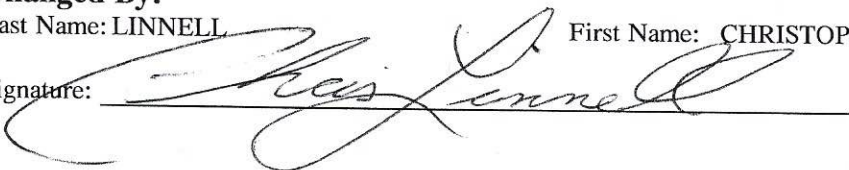

Badge No.: 128

Date: 08/04/2019