

Alcotest 7110 Calibration Record


Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01810 Calib. Date: 05/13/2020 Calib. No.: 00041
Certification File No.: 01776 Cert. Date: 11/27/2019 Cert. No.: 00031
Linearity File No.: 01777 Lin. Date: 11/27/2019 Lin. No.: 00031
Solution File No.: 01809 Soln. Date: 04/27/2020 Soln. No.: 00308
Sequential File No.: 01810 File Date: 05/13/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWL S3-0441
Control Solution %: 0.100% Expires: 10/14/2021
Solution Control Lot: 19270 Bottle No.: 0514

Coordinator

Last Name: WATSON First Name: MATTHEW MI: R
Signature: Tpr. J [Signature] #7078 Badge No.: 7078
Date: 05/13/2020

*Black Key Temperature Probe Serial.....# DDLBP3 - 0084 (MRW)
*Digital NIST Temperature Measuring System Serial.....# 191959028 (MRW)

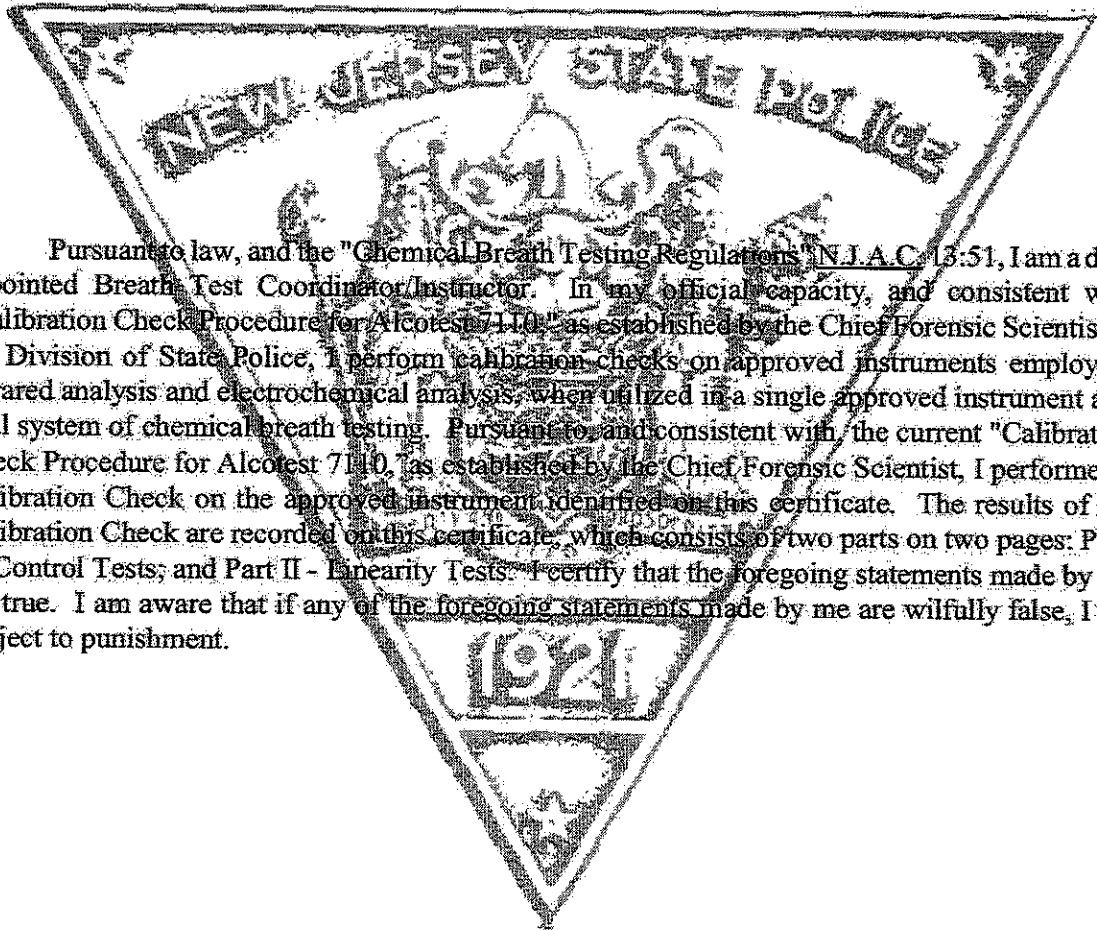

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110, as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	01810	Calib. Date:	05/13/2020
Certification File No.:	01811	Cert. Date:	05/13/2020
Linearity File No.:	01777	Lin. Date:	11/27/2019
Solution File No.:	01809	Soln. Date:	04/27/2020
Sequential File No.:	01811	File Date:	05/13/2020
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWL S3-0441
Solution Control Lot:	19270	Expires:	10/14/2021
		Bottle No.:	0514

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:02D		
Control 1 EC	0.099%	10:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04D		
Control 2 EC	0.097%	10:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05D		
Control 3 EC	0.097%	10:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07D		

All tests within acceptable tolerance.

Coordinator

Last Name: WATSON

First Name: MATTHEW


MI: R

Signature: Tpr. I Matthew A. Watson #7078

Badge No.: 7078

Date: 05/13/2020

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

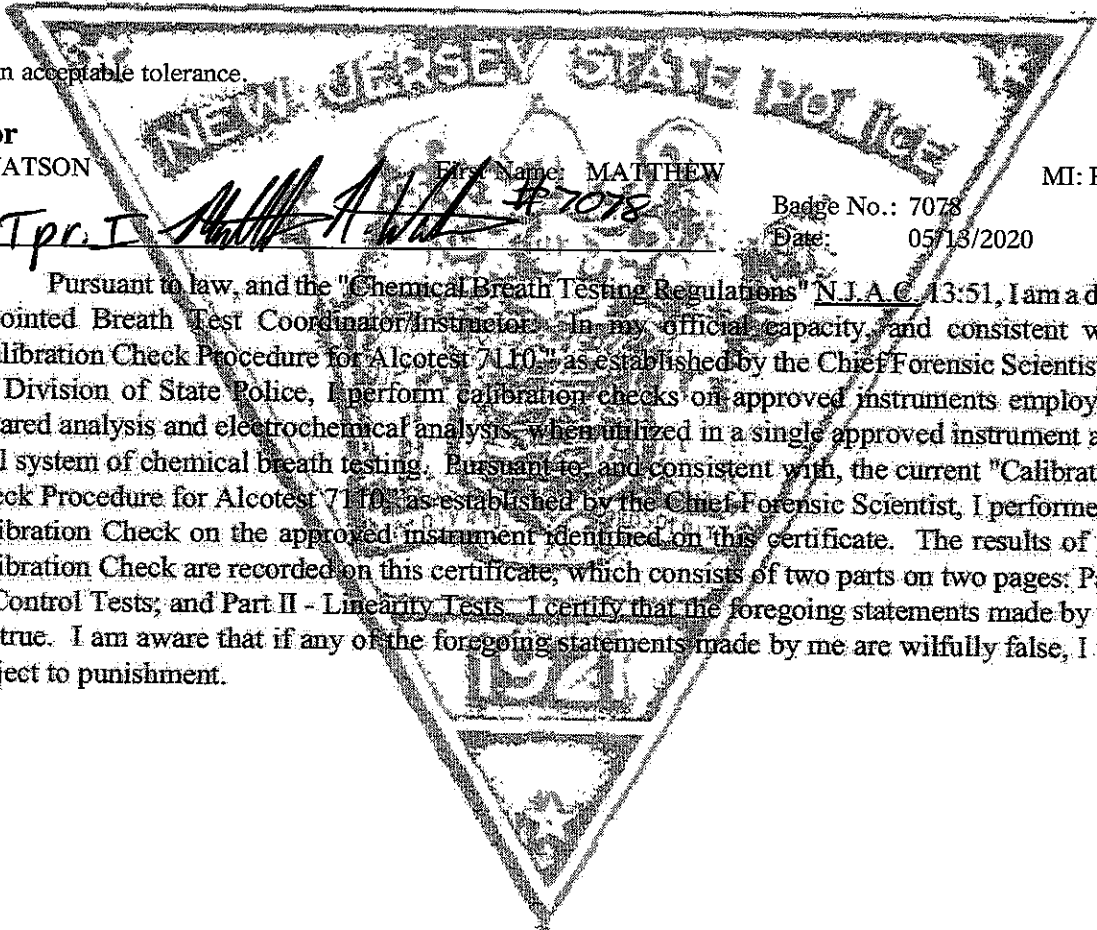

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWJ-0018
Location: SEASIDE HEIGHTS POLICE
Calibration File No.: 01810 **Calib. Date:** 05/13/2020 **Calib. No.:** 00041
Certification File No.: 01811 **Cert. Date:** 05/13/2020 **Cert. No.:** 00032
Linearity File No.: 01812 **Lin. Date:** 05/13/2020 **Lin. No.:** 00032
Solution File No.: 01809 **Soln. Date:** 04/27/2020 **Soln. No.:** 00308
Sequential File No.: 01812 **File Date:** 05/13/2020

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDRF S3-0009
Control Solution %: 0.040% **Expires:** 11/04/2021
Solution Control Lot: 19310 **Bottle No.:** 0498

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDCN-0054
Control Solution %: 0.080% **Expires:** 11/11/2021
Solution Control Lot: 19320 **Bottle No.:** 1176

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0261
Control Solution %: 0.160% **Expires:** 12/02/2021
Solution Control Lot: 19360 **Bottle No.:** 1296

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:16D		
Control 1 EC	0.040%	10:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.038%	10:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:18D		
Control 2 EC	0.040%	10:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.038%	10:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		
Control 3 EC	0.078%	10:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.077%	10:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22D		
Control 4 EC	0.078%	10:23D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.078%	10:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:24D		
Control 5 EC	0.156%	10:25D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.156%	10:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:27D		
Control 6 EC	0.156%	10:27D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.155%	10:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:29D		

All tests within acceptable tolerance.

Coordinator

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature: Tp.i. J. [Handwritten Signature]

[Handwritten Signature] #7078

Badge No.: 7078

Date: 05/13/2020

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	01810	Calib. Date:	05/13/2020
Certification File No.:	01811	Cert. No.:	00041
Linearity File No.:	01812	Cert. Date:	05/13/2020
Solution File No.:	01813	Lin. No.:	00032
Sequential File No.:	01813	Lin. Date:	05/13/2020
		Soln. No.:	00309
		File Date:	05/13/2020
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWL S3-0441
Solution Control Lot:	20090	Expires:	02/19/2022
		Bottle No.:	0177

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:33D		
Control 1 EC	0.098%	11:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:35D		
Control 2 EC	0.098%	11:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:36D		
Control 3 EC	0.099%	11:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DOWJP2-064 MRW

Changed By:

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature:  #7078

Badge No.: 7078

Date: 05/13/2020

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Tpr. I Matthew R. Watson
Name

7078
Badge No.

Location:

Seaside Heights Police
Agency

ARWJ-0018
Alcotest Serial No.

Equipment:

191959028
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDRF 53-0009	08:51 D	9:52 D	34.0°C
0.08%	DDCN-0054	08:51 D	9:53 D	34.0°C
0.10%	PDWL 53-0441	08:51 D	09:54 D	34.0°C
0.16%	DDWF 53-0261	08:51 D	09:55 D	34.0°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr. I [Signature] #7078
Coordinator's Signature

5/13/2020
Date



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.



- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:
DDRFS3-0009

Certification Date:
3.9.20

Technician:
M

Re-Certification Due Date:
3.9.21



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.


- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:
DDCN-0054

Certification Date:
3.10.20

Technician:
MB

Re-Certification Due Date:
3.10.21



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDWF S3- 0261

Certification Date:

Technician:

Re-Certification Due Date:

3-10-20

AK

3-10-21

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

Certification Date:

Next Certification Due:

DDLBP3-0084

3-11-20

3-11-21

Probe Value:

104

Dräger, Inc.

[Signature]



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177847

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 191959028 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Thermistor Module	A17118	20 Apr 2019	1000424560
Thermistor Module	A27129	10 Jan 2020	1000436202
Temperature Calibration Bath	A73332		
Temperature Probe	3039	08 May 2019	6-B7F4L-20-1
Temperature Calibration Bath	A79341		
Temperature Probe	5394	29 Jan 2020	B9124038
Temperature Calibration Bath	B16388		
Temperature Probe	5267	28 Jan 2020	B9124036

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 13 Feb 2019 Cal Due Date: 13 Feb 2021
 Test Conditions: 38.85%RH 24.21°C 1023mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		-0.002	0.001	Y	-0.052	0.048	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.001	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.000	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		100.000	100.003	Y	99.95	100.05	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded)- Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Aaron Justice

Aaron Justice, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
 Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-RVA.
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177847

Traceable® Certificate of Calibration for Digital Thermometer

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/21/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1232 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 14, 2021.


As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of October, 2019.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl-alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/14/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19310

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 04, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of November, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/20/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19320

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0971 to 0.0985 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 11, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of November, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 12/11/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1956 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 02, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18 day of December, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 382-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 03/03/2020

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 20090


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1200 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 19, 2022.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 3 day of March, 2020.
Notary

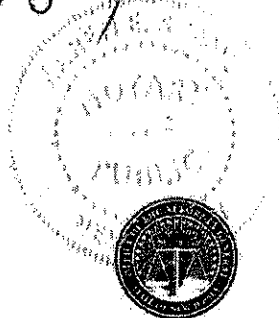

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024

An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Water and Public Safety
This is to certify that

Matthew R. Watson
New Jersey State Police



IS QUALIFIED AND COMPETENT TO CONDUCT OPERATIONS AS DESCRIBED HEREIN PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcoquest 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 10th DAY OF August

TWO THOUSAND AND 10th

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY


ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-8-12	GCPA	WIM Long
2. 7/14/15	CMPA	Adam Gander
3. 3/23/17	Lakehurst	Michelle Jemelny
4. 9-20-19	GCPA	WIM Long
5.		
6.		
7.		
8.		
9.		

S.P. 2935 (Rev. 03/10)

DEPARTMENT OF
Water and Public Safety
This is to certify that

Matthew R. Watson
Breath Test Courtroom Instructor



IS QUALIFIED AND COMPETENT TO CONDUCT OPERATIONS AS DESCRIBED HEREIN PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcoquest 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Sixteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ACTING ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2935 (Rev. 03/13)

Dräger

Alcotest® 7110 MKII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKII-C has been tested for accuracy and found to be in accordance with the Federal Highway Dept. Safety Administration Standard for roadside breath testing devices. The Alcotest MKII-C is certified as a "Model" and "Prototype" EBT with 40 cc alcohol, 30 ppm BAC and 0.10% alcohol. The manufacturer recommends accuracy verification of this instrument within 30 minutes of the calibration date below, or sooner, according to your State Specifications.

Calibration Date:

10-12-16

SERIAL NUMBER

ARWJ-0018

Dräger Safety Diagnostics, Inc.

AC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDWLS3-0441

Certification Date:

3-9-20

Technician:

AM / M.B.

Re-Certification Due Date:

3-9-21

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDWJP2-064

Certification Date:

3-9-20

Next Certification Due:

3-9-21

Probe Value:

100

Draeger, Inc.

[Signature]