

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE		
Calibration File No.:	01810	Calib. Date:	05/13/2020
Certification File No.:	01811	Cert. Date:	05/13/2020
Linearity File No.:	01812	Lin. Date:	05/13/2020
Solution File No.:	01846	Soln. Date:	09/21/2020
Sequential File No.:	01846	File Date:	09/21/2020
		Calib. No.:	00041
		Cert. No.:	00032
		Lin. No.:	00032
		Soln. No.:	00320

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWL S3-0441
Control Solution %:	0.100%			Expires:	07/06/2022
Solution Control Lot:	20320			Bottle No.:	0235

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:28D		
Control 1 EC	0.100%	09:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30D		
Control 2 EC	0.098%	09:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31D		
Control 3 EC	0.098%	09:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33D		

All tests within acceptable tolerance.

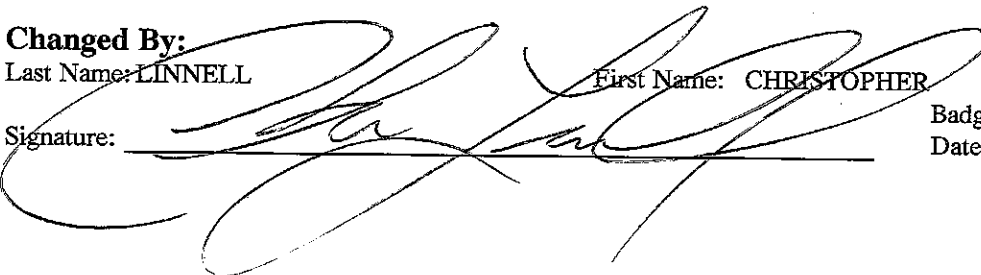
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 09/21/2020