

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01848	Calib. Date: 09/29/2020
Certification File No.:	01849	Calib. No.: 00042
Linearity File No.:	01850	Cert. Date: 09/29/2020
Solution File No.:	01858	Cert. No.: 00033
Sequential File No.:	01858	Lin. Date: 09/29/2020
		Lin. No.: 00033
		Soln. Date: 11/03/2020
		Soln. No.: 00322
		File Date: 11/03/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWL S3-0440
Solution Control Lot:	20320	Expires: 07/06/2022
		Bottle No.: 0580

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:26S		
Control 1 EC	0.098%	15:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	15:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:27S		
Control 2 EC	0.097%	15:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	15:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:29S		
Control 3 EC	0.097%	15:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:30S		

All tests within acceptable tolerance.

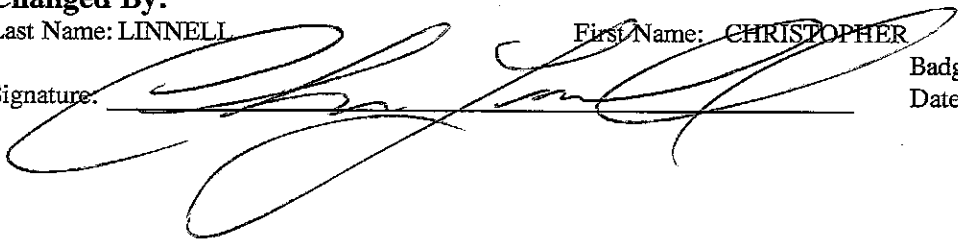
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 11/03/2020