

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWJ-0018
Location:	SEASIDE HEIGHTS POLICE	
Calibration File No.:	01975	Calib. Date: 01/20/2022
Certification File No.:	01976	Calib. No.: 00045
Linearity File No.:	01977	Cert. Date: 01/20/2022
Solution File No.:	02001	Cert. No.: 00036
Sequential File No.:	02001	Lin. Date: 01/20/2022
		Lin. No.: 00036
		Soln. Date: 03/13/2022
		Soln. No.: 00345
		File Date: 03/13/2022

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWL S3-0441
Control Solution %:	0.100%			Expires:	12/28/2023
Solution Control Lot:	21480			Bottle No.:	0496

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:35S		
Control 1 EC	0.101%	10:36S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:36S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:37S		
Control 2 EC	0.099%	10:37S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:37S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		
Control 3 EC	0.098%	10:39S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:39S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: \_\_\_\_\_

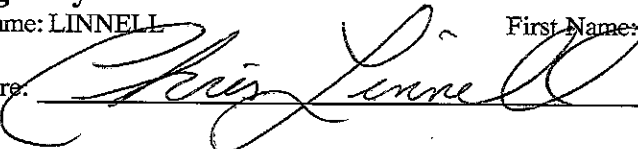

Badge No.: 128

Date: 03/13/2022