

Calibrating Unit New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: SEASIDE HEIGHTS POLICE
Serial No.: ARWJ-0018
Calibration File No.: 02070
Calib. Date: 07/15/2022
Calib. No.: 00046
Certification File No.: 02071
Cert. Date: 07/15/2022
Cert. No.: 00037
Linearity File No.: 02072
Lin. Date: 07/15/2022
Lin. No.: 00037
Solution File No.: 02100
Soln. Date: 09/26/2022
Soln. No.: 00355
Sequential File No.: 02100
File Date: 09/26/2022

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 21480
Model No.: CU-34
Serial No.: DDWL S3-0440
Expires: 12/28/2023
Bottle No.: 0541

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:05D		
Control 1 EC	0.102%	21:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	21:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:07D		
Control 2 EC	0.101%	21:07D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	21:07D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:08D		
Control 3 EC	0.101%	21:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	21:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:10D		

All tests within acceptable tolerance.

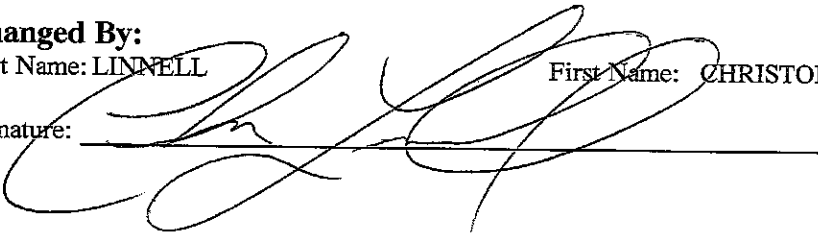
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LINNELL

First Name: CHRISTOPHER

MI: J

Signature: 

Badge No.: 128

Date: 09/26/2022